


## Supplementary Figure 8

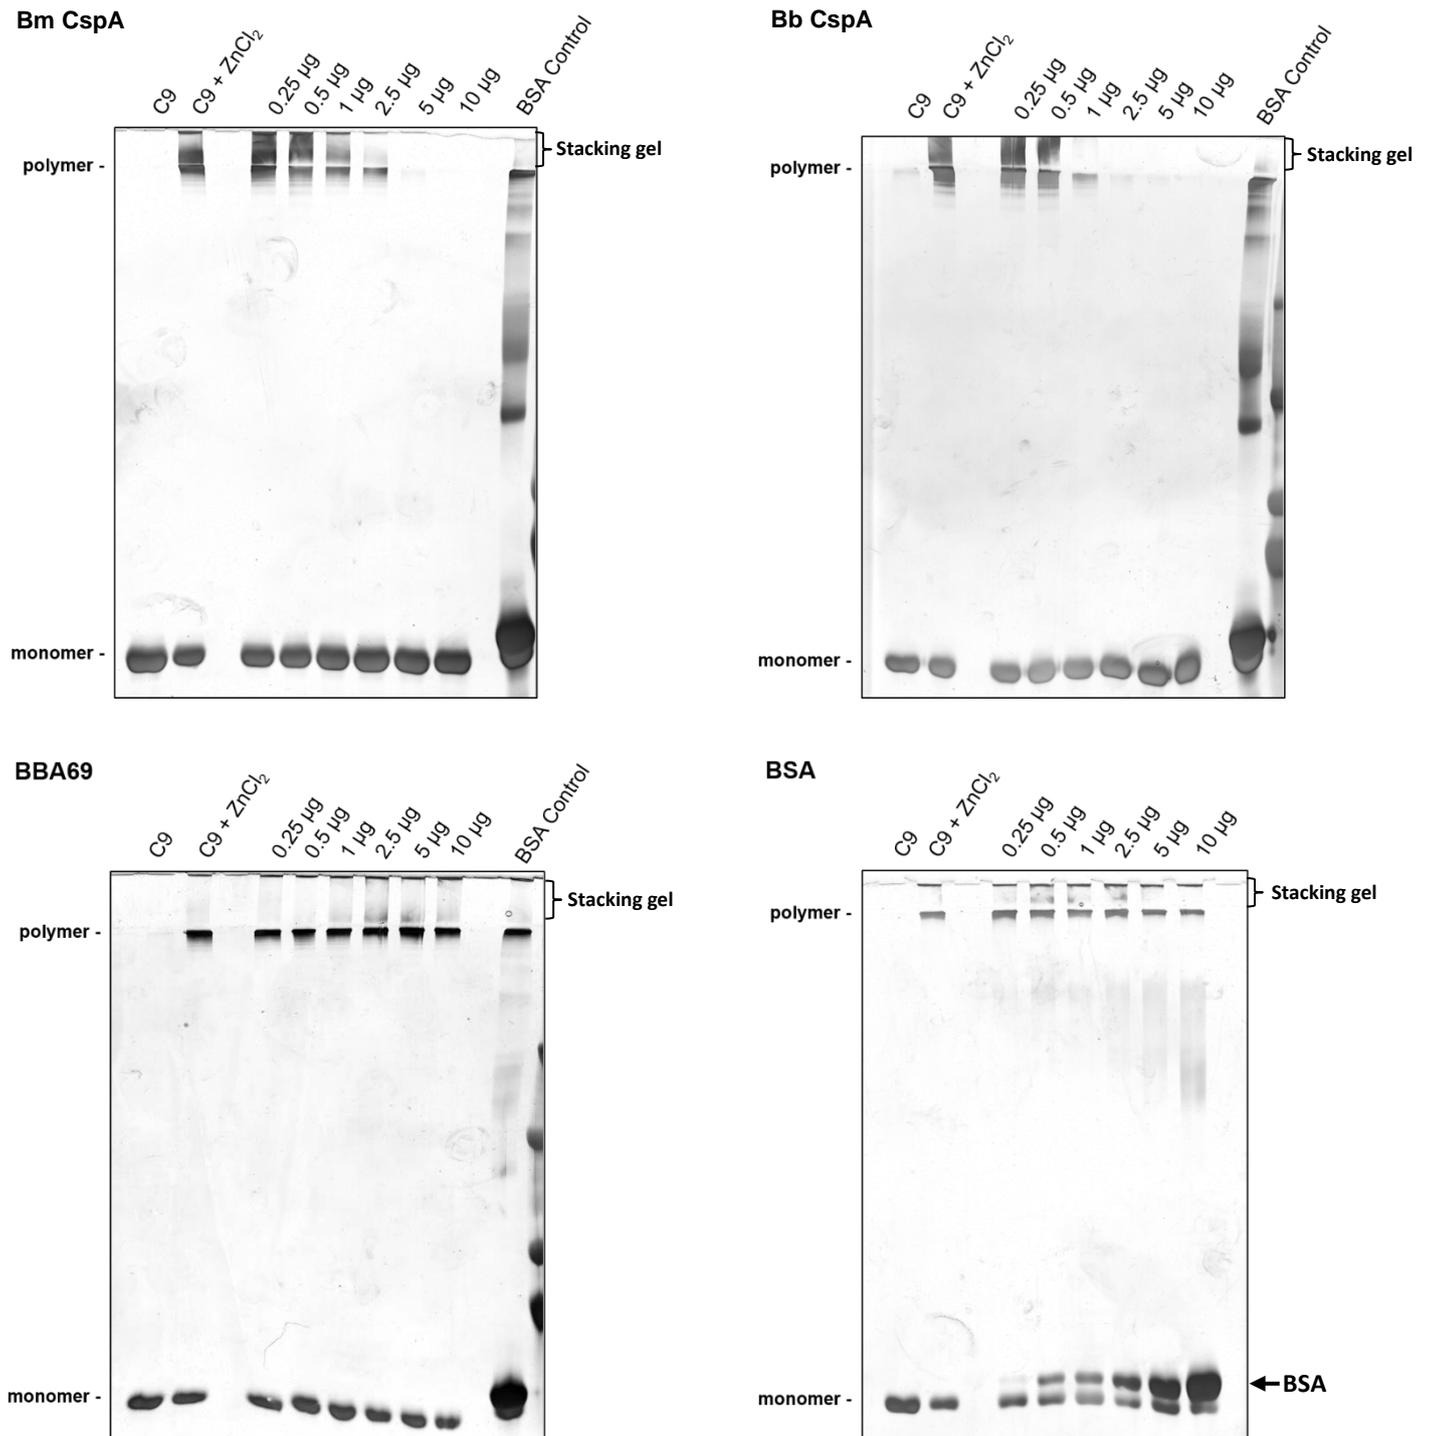

**Uncropped silver-stained gels of figure 7E.** SDS polyacrylamide gels stained with silver were scanned by a GS-710 Imaging Densitometer (Bio-Rad) and for image processing the Quantity One 4.2.1 software (Bio-Rad) was used. The general settings were as follows:

- Application: Gel
- Filter: Silver stain
- Resolution: 42,3 \* 42,3 microns =High for small gels with tiny features
- Transform operations of the silver stained gel: high: 4095; low: 0; gamma: 1.00